







KEYBOARD



PIRANT
PORT

OPEN



CLOSE

VENT VALVE

QUICK



SLAM

ENABLE



DISABLE



PRESSURE
GAUGE
OUTPUT





PURGE GAS 5 GAS 4 GAS 3 GAS 2 GAS 1

He	O ₂	Ar	10%	50%	100%
100000	100000	100000	100000	100000	100000

DANGER
HIGH VOLTAGE

DANGER



DANGER
HIGH VOLTAGE

DANGER
HIGH VOLTAGE
UP TO 100 kV

LIFTING MACHINE BY CRACKING TUBE
WILL RESULT IN SERIOUS DAMAGE

STAND BY
N₂ 15 PSI

NOTICE
DO NOT
OPERATE
WITHOUT
TRAINING
PERSONNEL


COOLANT
OUT
1/4" NPT

COOLANT
IN
1/4" NPT




FIELD EVALUATED
**To Recognized
National Standards**
167268

NOTICE




This equipment is manufactured
under one or more of the
following patents:

5,672,239	4,984,954
4,867,631	4,790,258
4,780,169	4,720,628
4,585,920	4,585,516
4,579,618	4,464,223



PETALUMA,
CALIFORNIA
MADE IN USA

Item : CS900
S/N : CS11522
Volt : 200/208 VAC
Curr : 30 Amps
Phase : 1
Freq : 50/60 Hz
Wires : 2 + Ground
Mfg : 6/2000

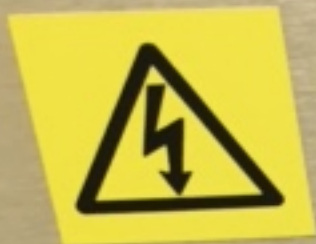

DANGER
HIGH VOLTAGE

DANGER
HIGH VOLTAGES
UP TO 240 VAC


DANGER
HAZARDOUS AREA, TRAINED
SERVICE PERSONNEL ONLY

POWER REQUIREMENTS
208VAC 25A 1Pn 50/60 Hz
(2-Wire + GND)

ETD To document
Reference Standards
ET298

NOTICE
Legal
This equipment is manufactured
under ISO 9001:2015 and ISO
14001:2015
Model: 1000-0000
Serial: 1000-0000
Date: 10/10/2020


DANGER
RF may be exposed
if safety interlock
switches are
bypassed without
disabling AC to RF
generator




30 AMP	5 AMP	5 AMP	50 AMP	10 AMP
CB1	CB2	CB3	CB4	CB5
MAIN	CONTROL	DC	RF	HEATER

115 VAC 1 AMP

115-MAIN POWER
200-240 VAC
50/60 HZ

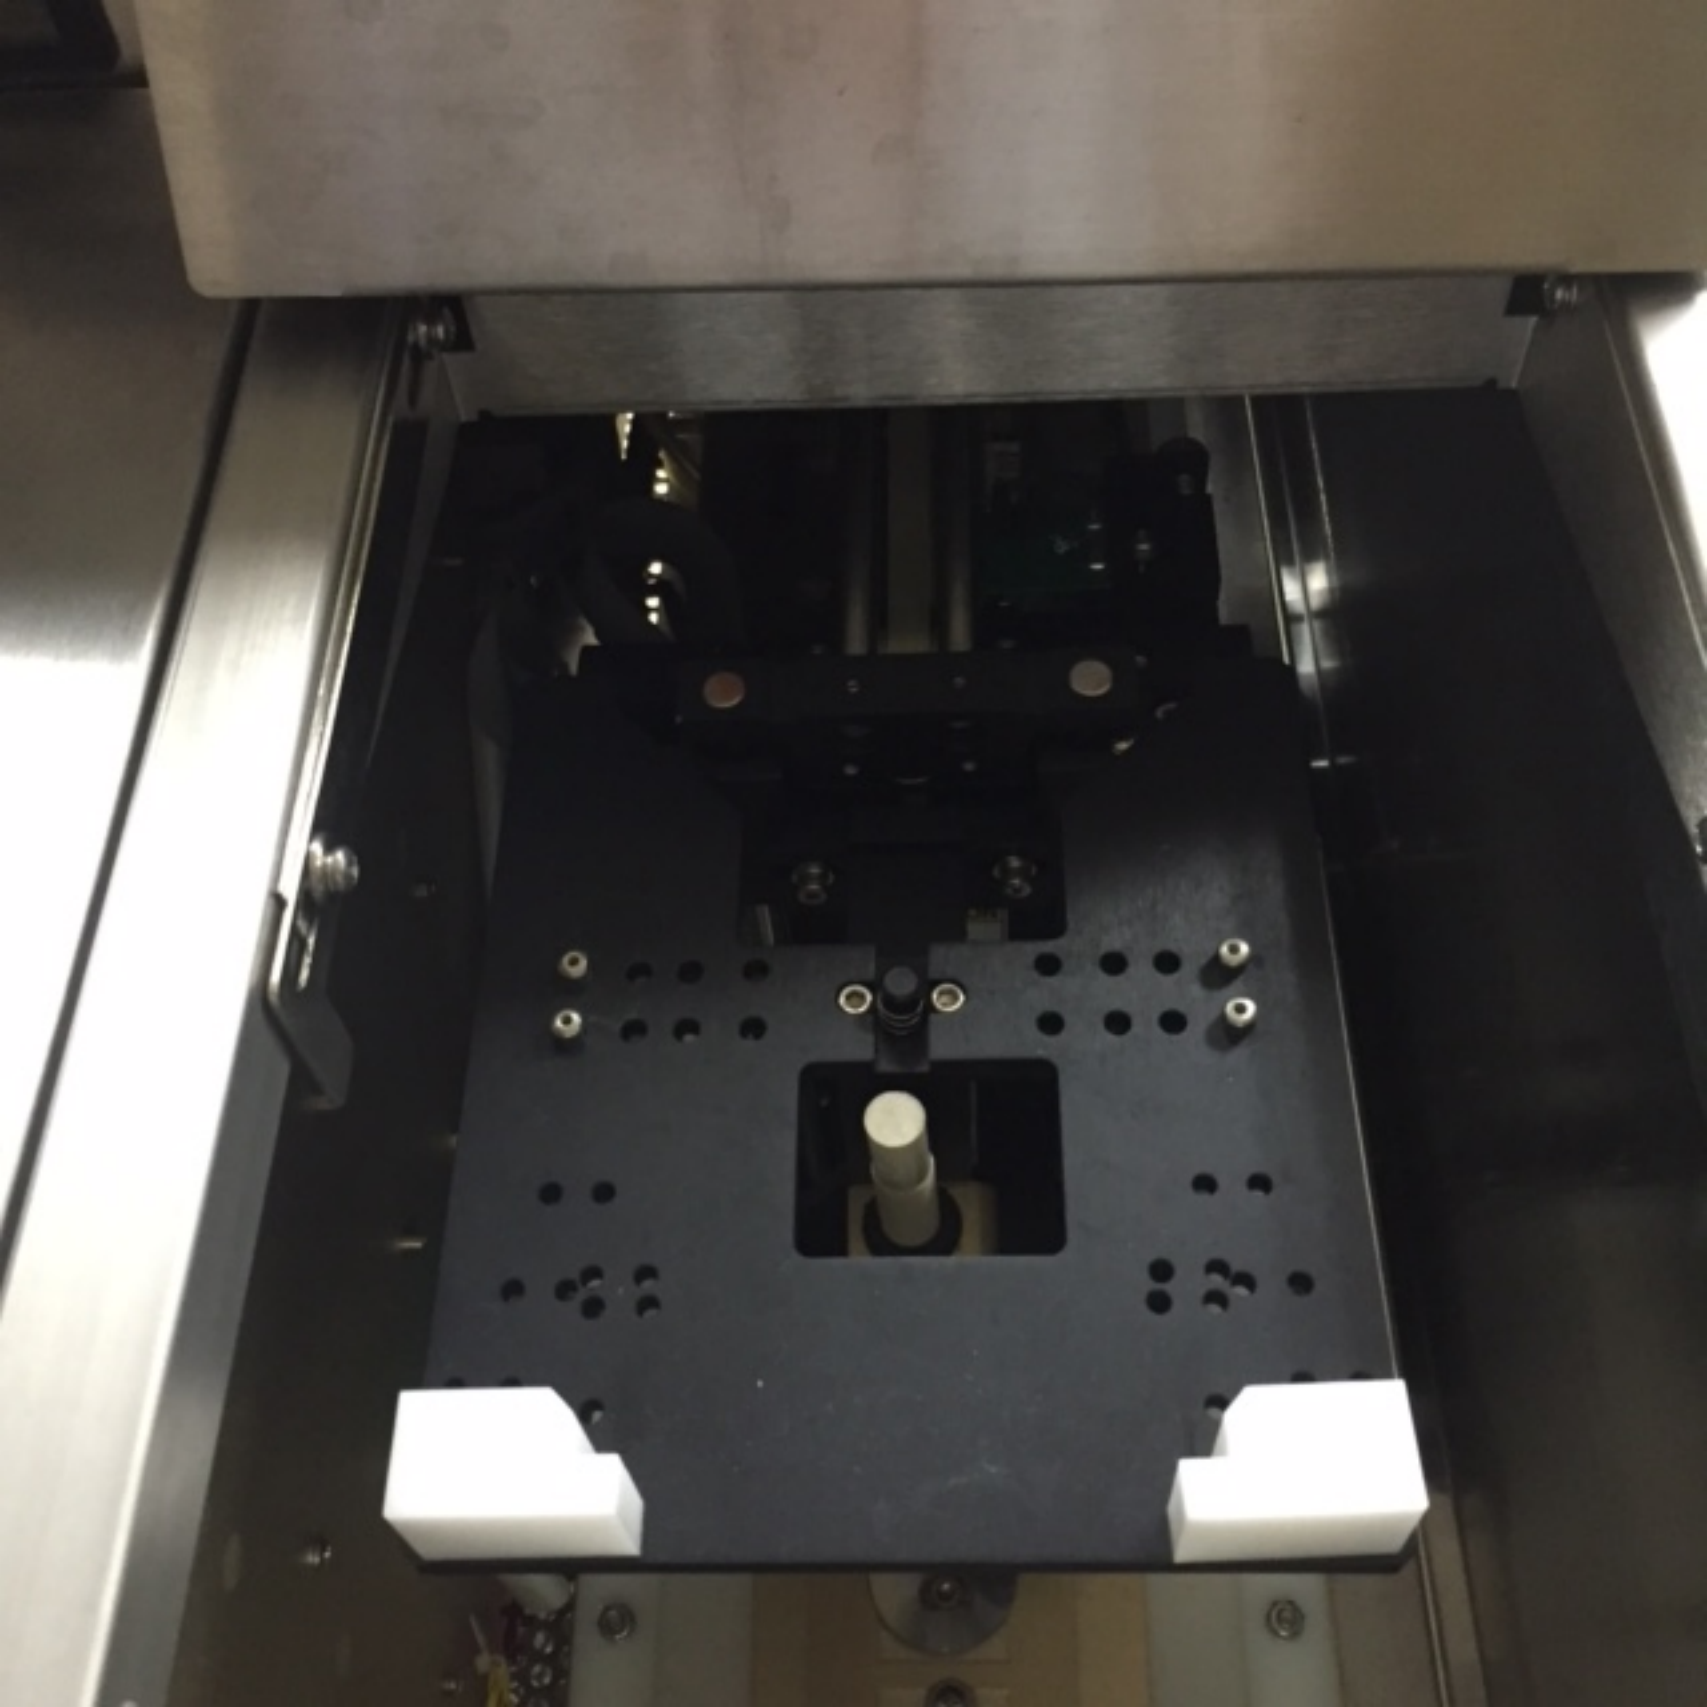

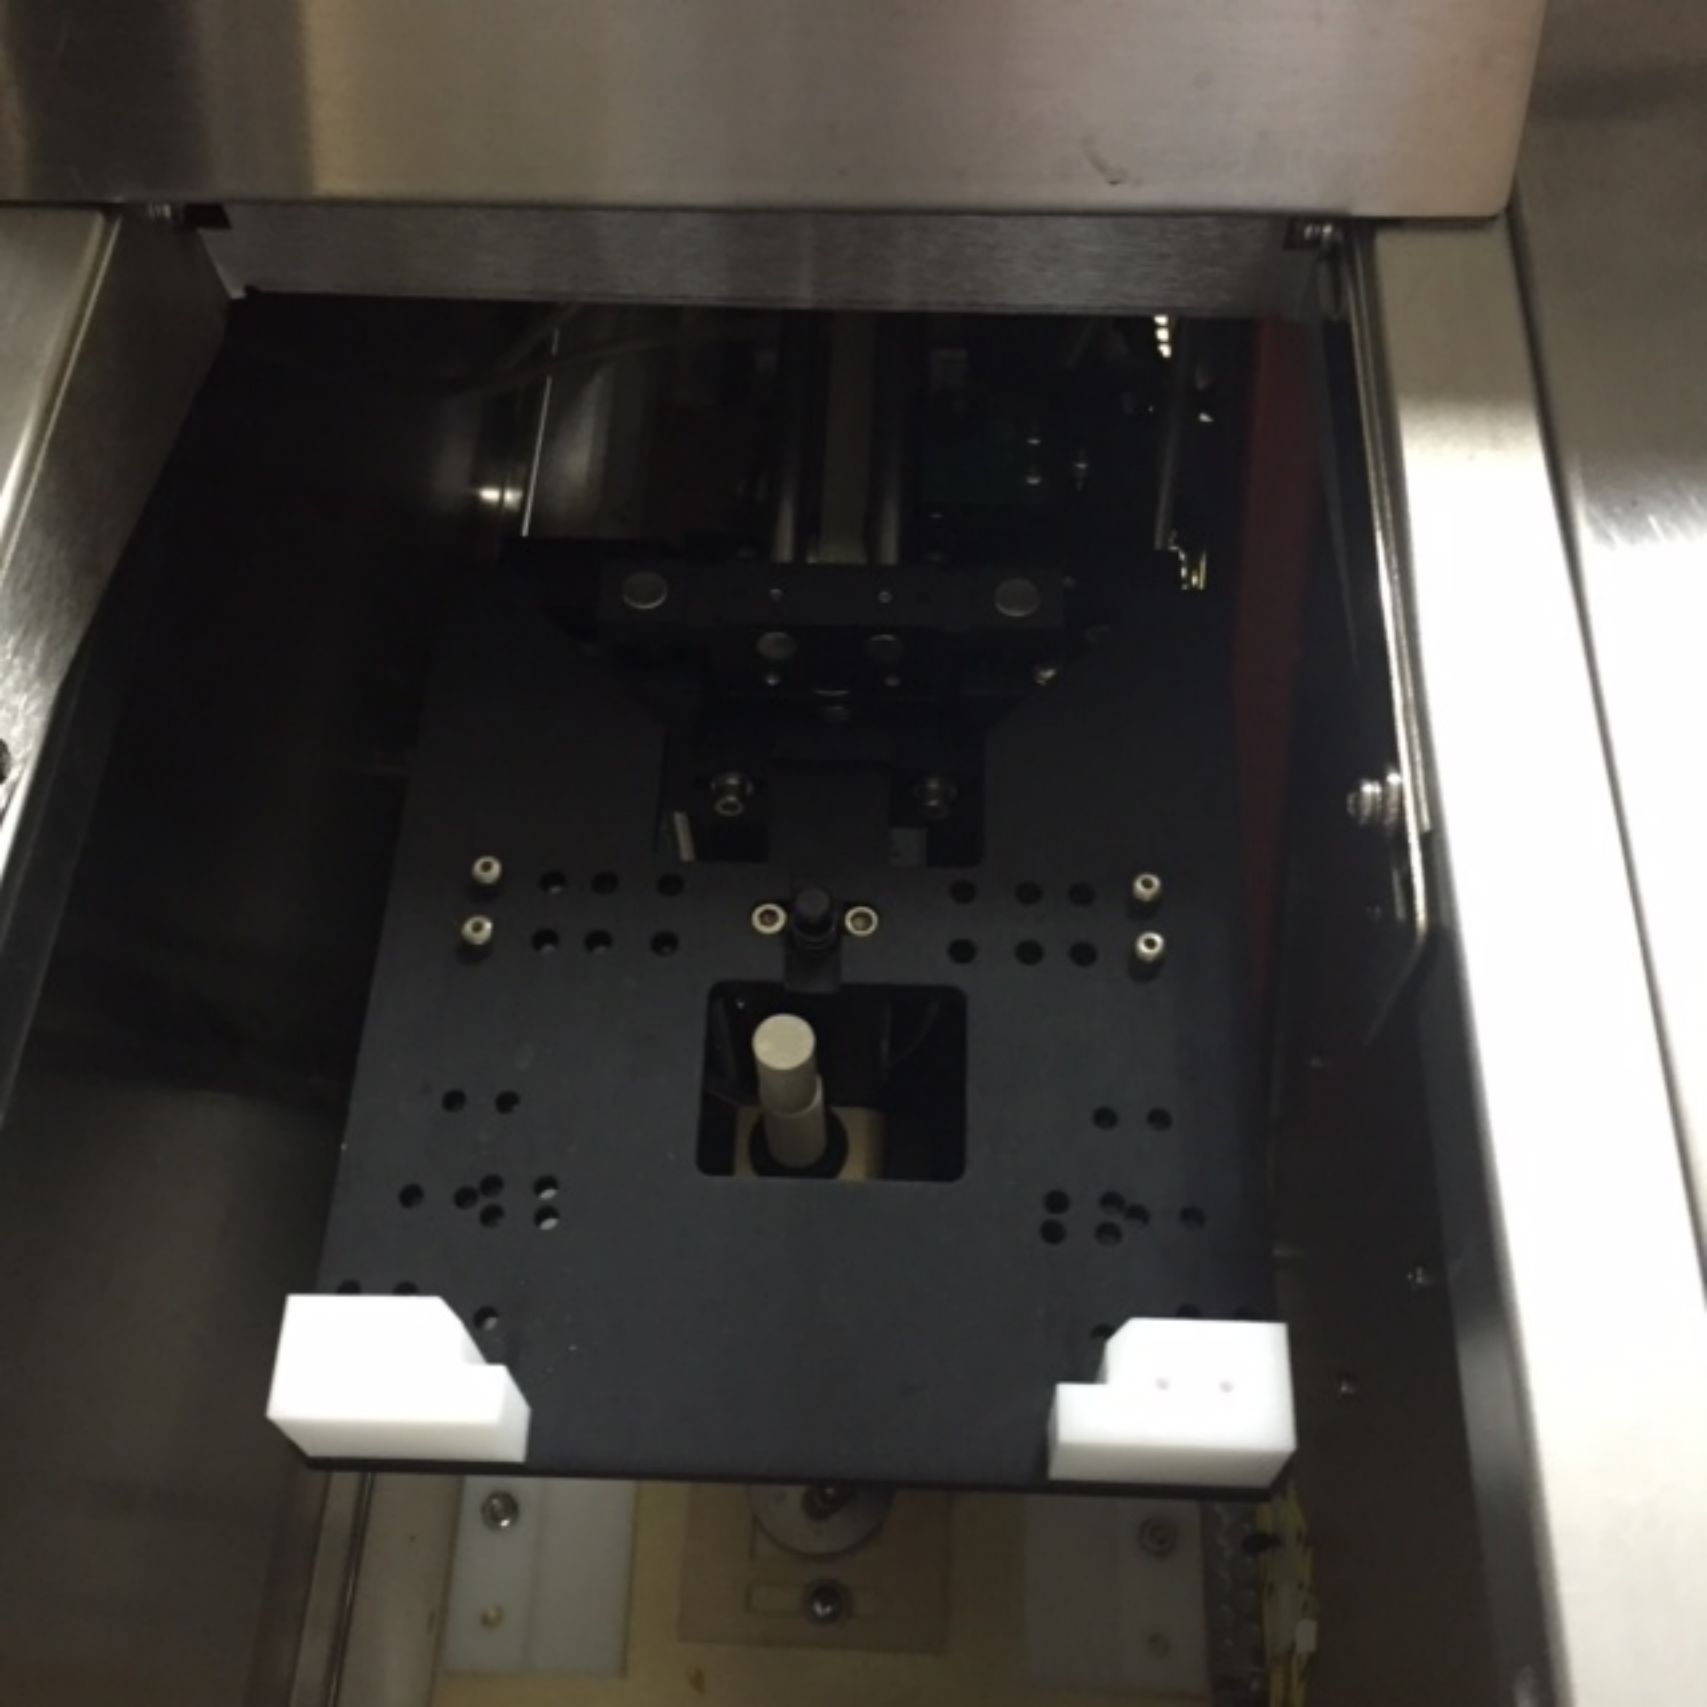

Operate system
Turn on exhaust
reaction chamber
Wear protective
handling chamber
surfaces. Consult
section of technical
observe company
procedure during op
and maintenance.



SLOW


DISABLE

RF ON HOURS
SINCE LAST CLEAN

RESET

RESSURE
GAUGE
OUTPUT

+

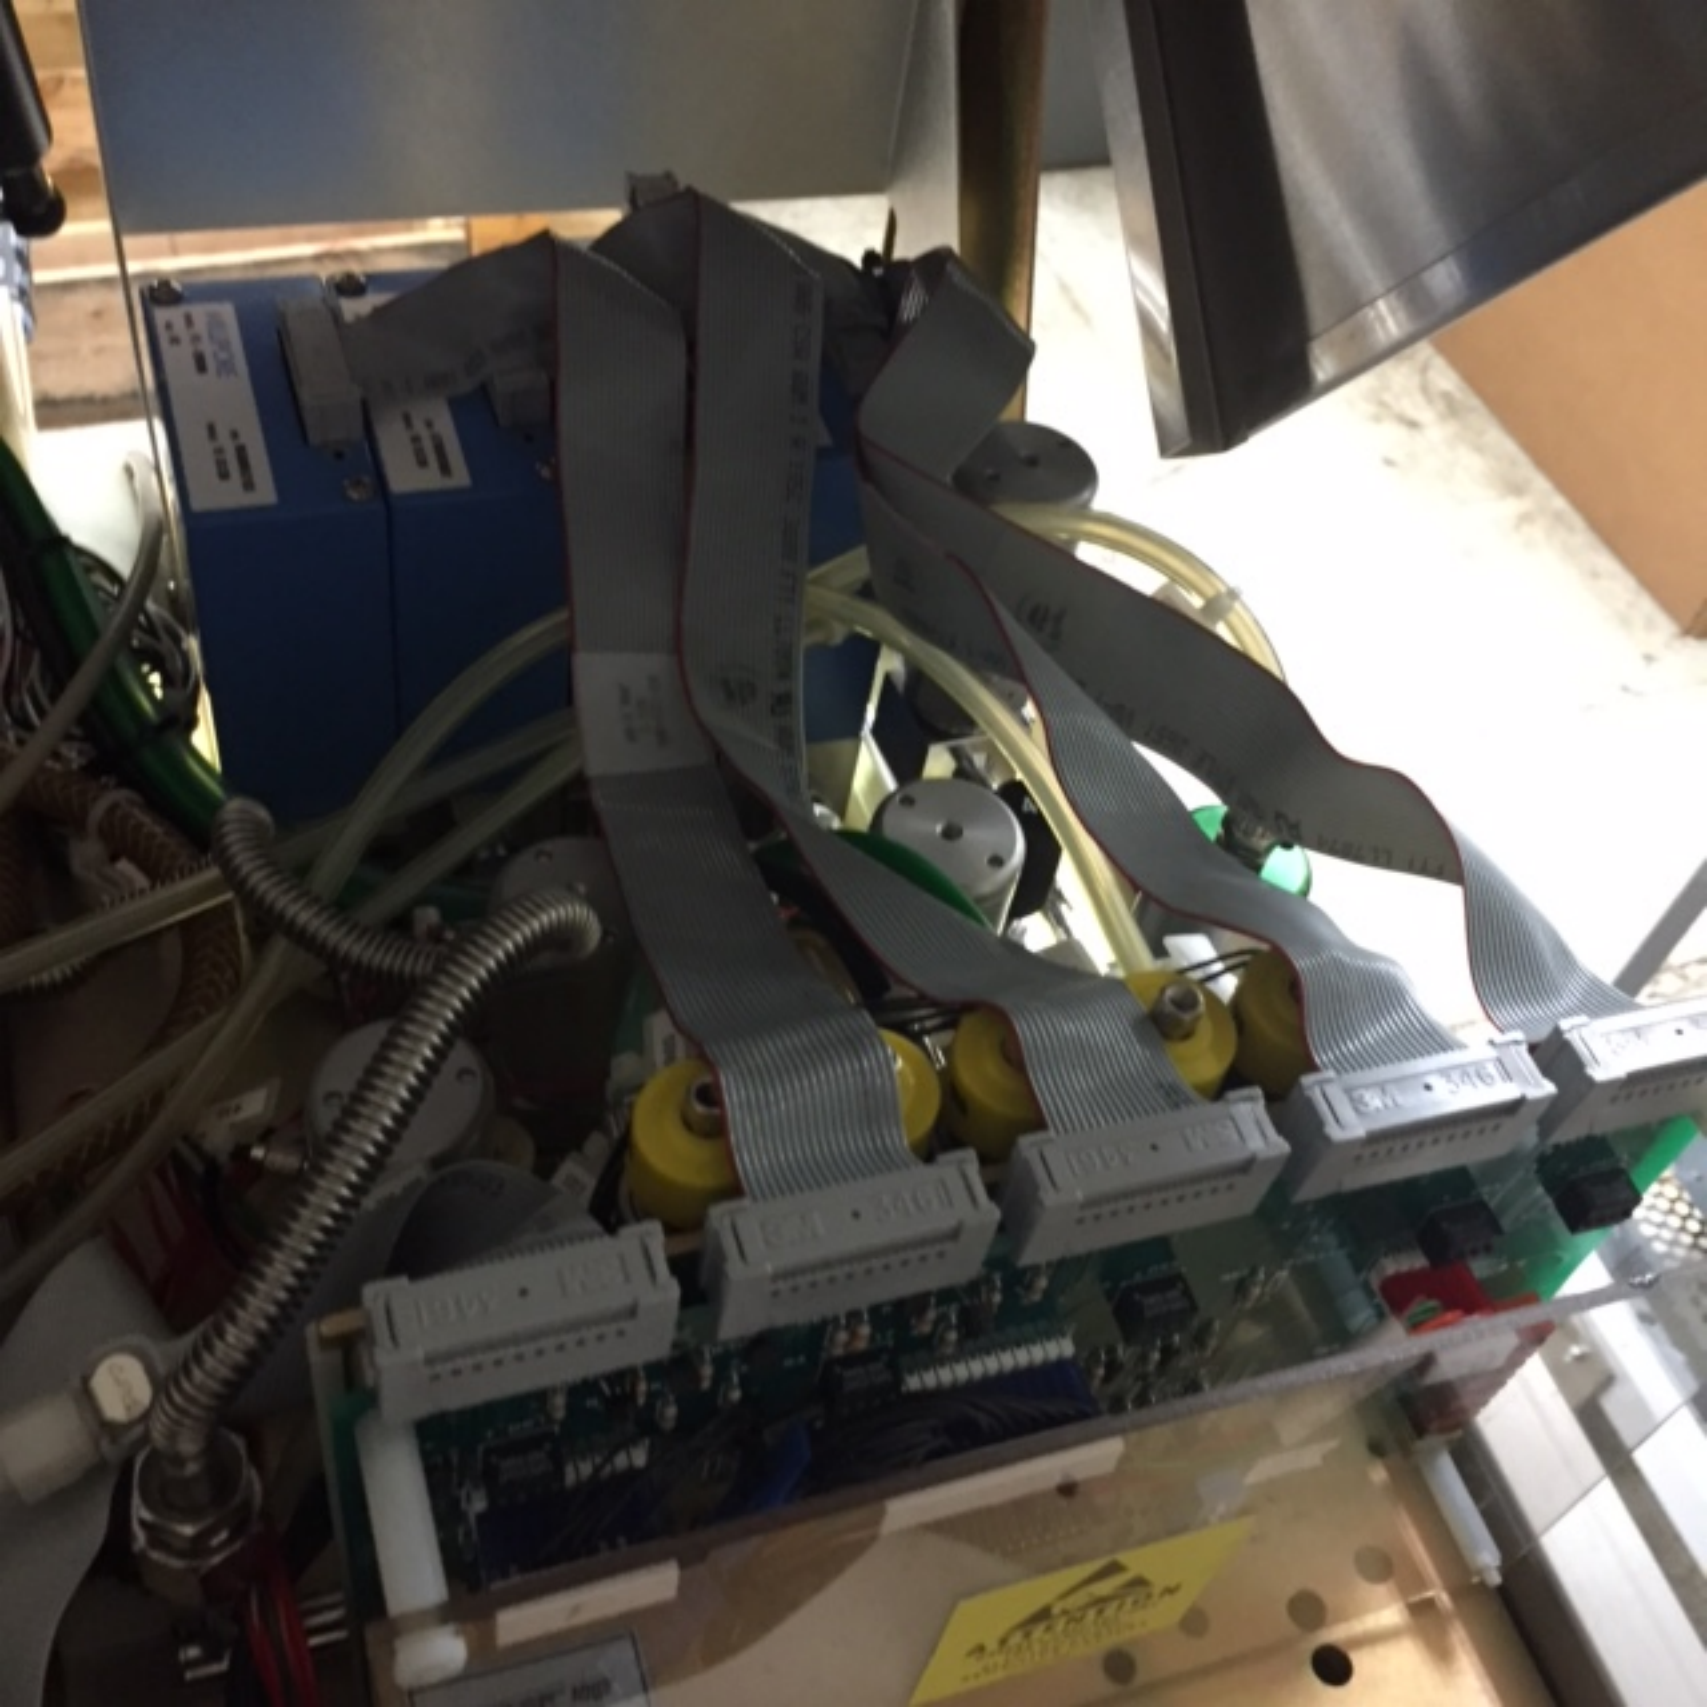



00-1071-00

UPC: 811
Q15 : 0
NAME :
SN : 101

MILLIPORE
MODEL FC-2500M
SERIAL 102

MILLIPORE
MODEL FC-2500M
SERIAL 102

SN A10000002
NAME 10 SCCM

SN 0000000102
NAME 10 SCCM

PURGE

N₂

15 PSIG

GAS 5

O₂

15 PSIG

GAS 4

He

15 PSIG

GAS 3

SF₆

15 PSIG

GAS 2

CHF₃

15 PSIG

GAS 1

N₂

15 PSIG

42 323 001 8

LIFTING MACHINE BY VACUUM TUBE
WILL RESULT IN SERIOUS DAMAGE

STAND BY
N₂ 15 PSI

NOTICE

legal

Legal Notice
This equipment is the property of the University of California, Los Angeles (UCLA) and is loaned to you for your use only. It is not to be sold, transferred, or otherwise disposed of without the written consent of the UCLA Office of the Vice President for Research and Innovation. Any unauthorized use or disposal of this equipment may result in legal action against you and your institution.

COOLANT OUT